

prepDATA2

User Manual

Version 1.4

2026-04-10



Table of Contents

- 1. GETTING STARTED.....3
 - 1.1 Overview 3
 - 1.2 Installation 3
 - 1.3 Uninstallation..... 3
 - 1.4 Start the Application 3
- 2. MAIN WINDOW.....4
 - 2.1 Docking and Layout 4
- 3. OPEN DATA FROM DRIVE.....5
 - 3.1 Select File..... 5
 - 3.2 Select Data..... 6
- 4. OPEN DATA FROM PREPASH7
 - 4.1 Select prepASH..... 7
 - 4.2 Select Data..... 8
- 5. LIVE WATCH9
- 6. CHART10
 - 6.1 Select Samples 10
 - 6.2 Zoom and Scroll 11
- 7. RESULT.....12
 - 7.1 Result Editor..... 12
 - 7.2 Result Table 13
- 8. STATISTIC.....14
 - 8.1 Statistic Editor 14
 - 8.2 Statistic Table..... 15
- 9. EXPORT TO EXCEL16
- 10. REPORT17
- 11. SAMPLELIST EDITOR18
 - 11.1 Create new Samplelist 18
 - 11.2 Export Samplelist 19
 - 11.3 Import Samplelist..... 20
- 12. PREPSTATION 2.0.....21
 - 12.1 Setup the Balance 22
 - 12.2 Setup the Rotary Unit..... 23
 - 12.3 Adjusting the Rotary Unit 24
 - 12.4 Weighing-in 26
- 13. AUDIT TRAIL VIEWER.....28
 - 13.1 Import 28
 - 13.2 Export 29
 - 13.3 Filtering..... 29

1. Getting Started

Please be aware that the prepDATA 2.0 is only compatible with prepASH 2.0. Previous prepASH models are not compatible and need the previous prepDATA version (available on www.precisa.com).

prepDATA2 is designed for Windows 7 / 8 / 10 and Windows 11, all with 32-bit or 64-bit support.

The software prepDATA enables comprehensive data analysis of your results.

1.1 Overview

prepDATA offers the following functions:

- Search and filter data from prepASH or drive
- Customize visualizations using docking windows
- Monitor the analysis process in real time
- Define additional results and statistics groups
- Export data to an Excel file. Microsoft Excel does not need to be installed
- Create custom reports
- Create and edit sample lists
- Create a weighingin lists with the prepSTATION

1.2 Installation

1. Unzip the file (e.g. setup_prepDATA2_V1_0_4.zip)
2. Run the file (e.g. setup_prepDATA2_V1_0_4.exe)
3. Follow the on-screen instructions

1.3 Uninstallation



Type "Uninstall prepDATA2" into the Windows search bar and press Enter key.

1.4 Start the Application

Type "prepDATA2" into the Windows search bar and press Enter key or double-clicking the prepDATA2 desktop icon to start the application.




2. Main Window


When the application starts, the prepDATA2 window is displayed.

2.1 Docking and Layout

The application allows you to organize and group the dock panels freely by dragging and dropping them, enabling a customized workspace layout.

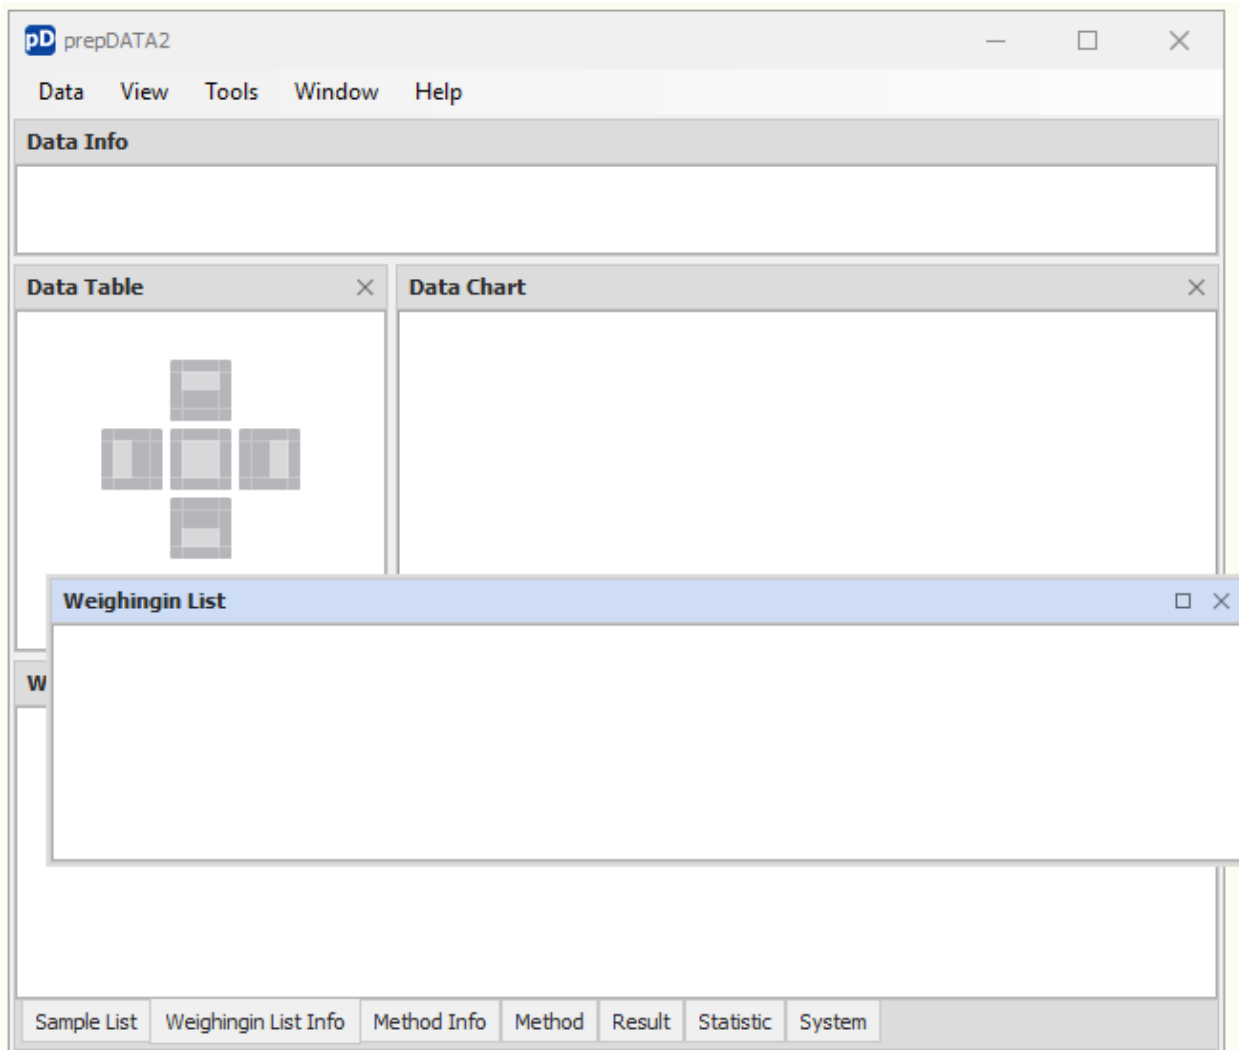


In the Window menu, click on **Set Default Layout** to restore the default view.

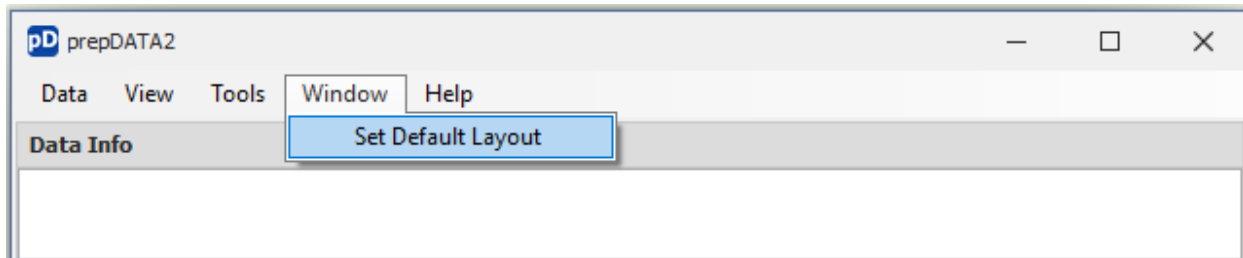


3. Open Data from Drive

To open data from the drive, navigate to the **Data** menu and select **Open from Drive**.

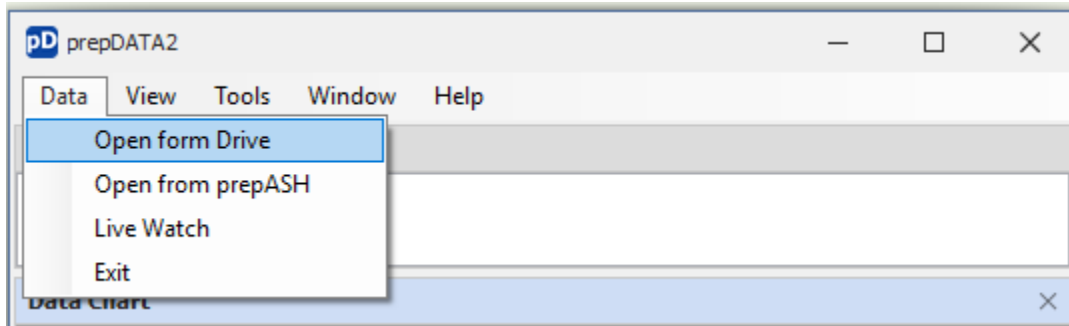

3.1 Select File

In the Open from Drive window, select a file with the extension *_analyses.dat* or *_backup.dat*, and then click on **Open**. The Select Data windows opens.

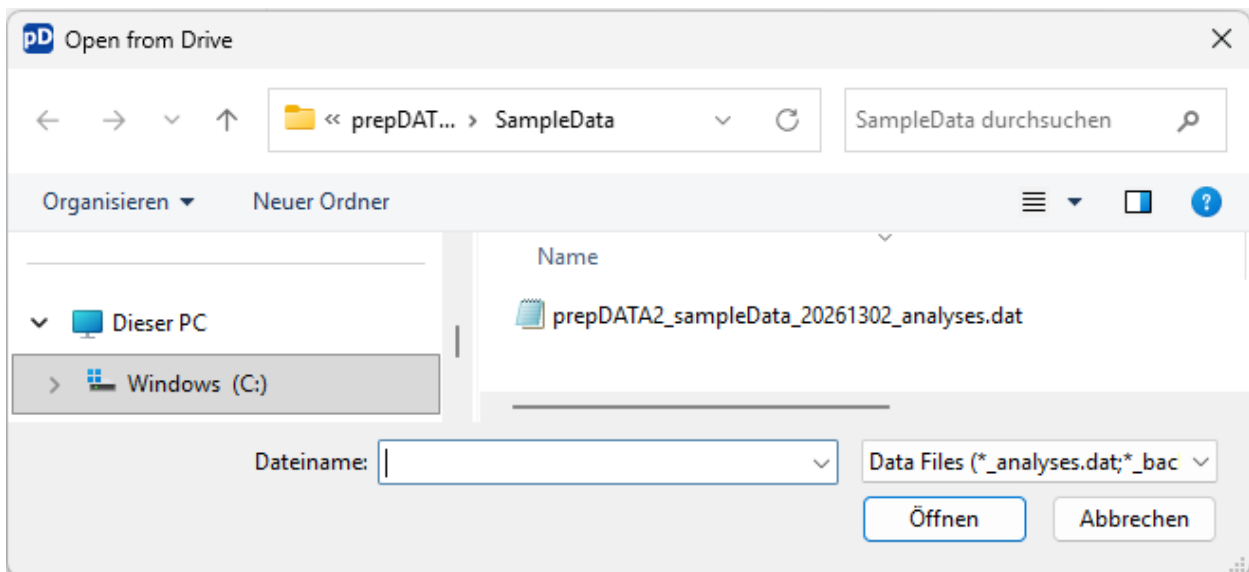


Hint


The installer package (e.g. *setup_prepDATA2_V1_0_4.zip*) contains a sample data file, located in the sample data folder.

3.2 Select Data

In the Select Data window, select an analysis and click on **Select**.

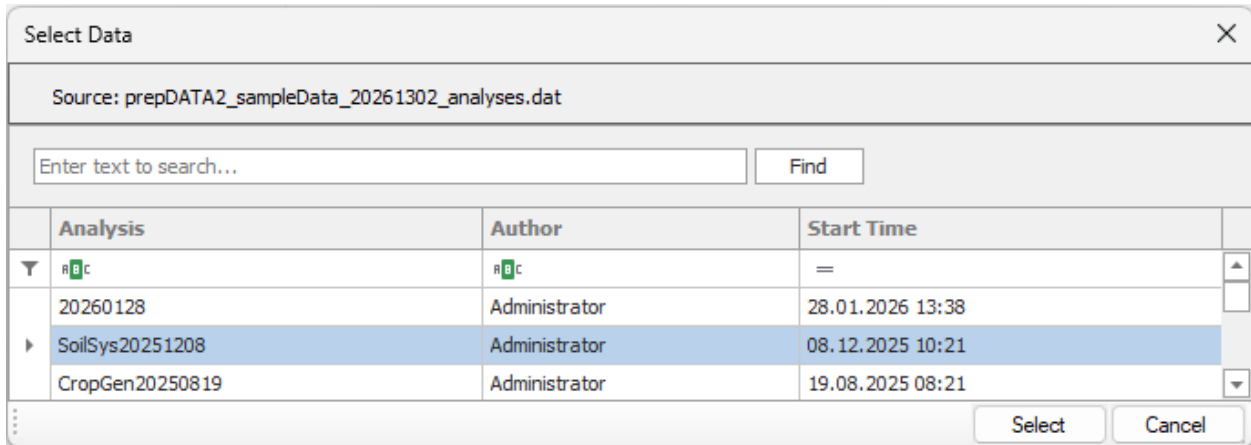


The selected analysis is now displayed.

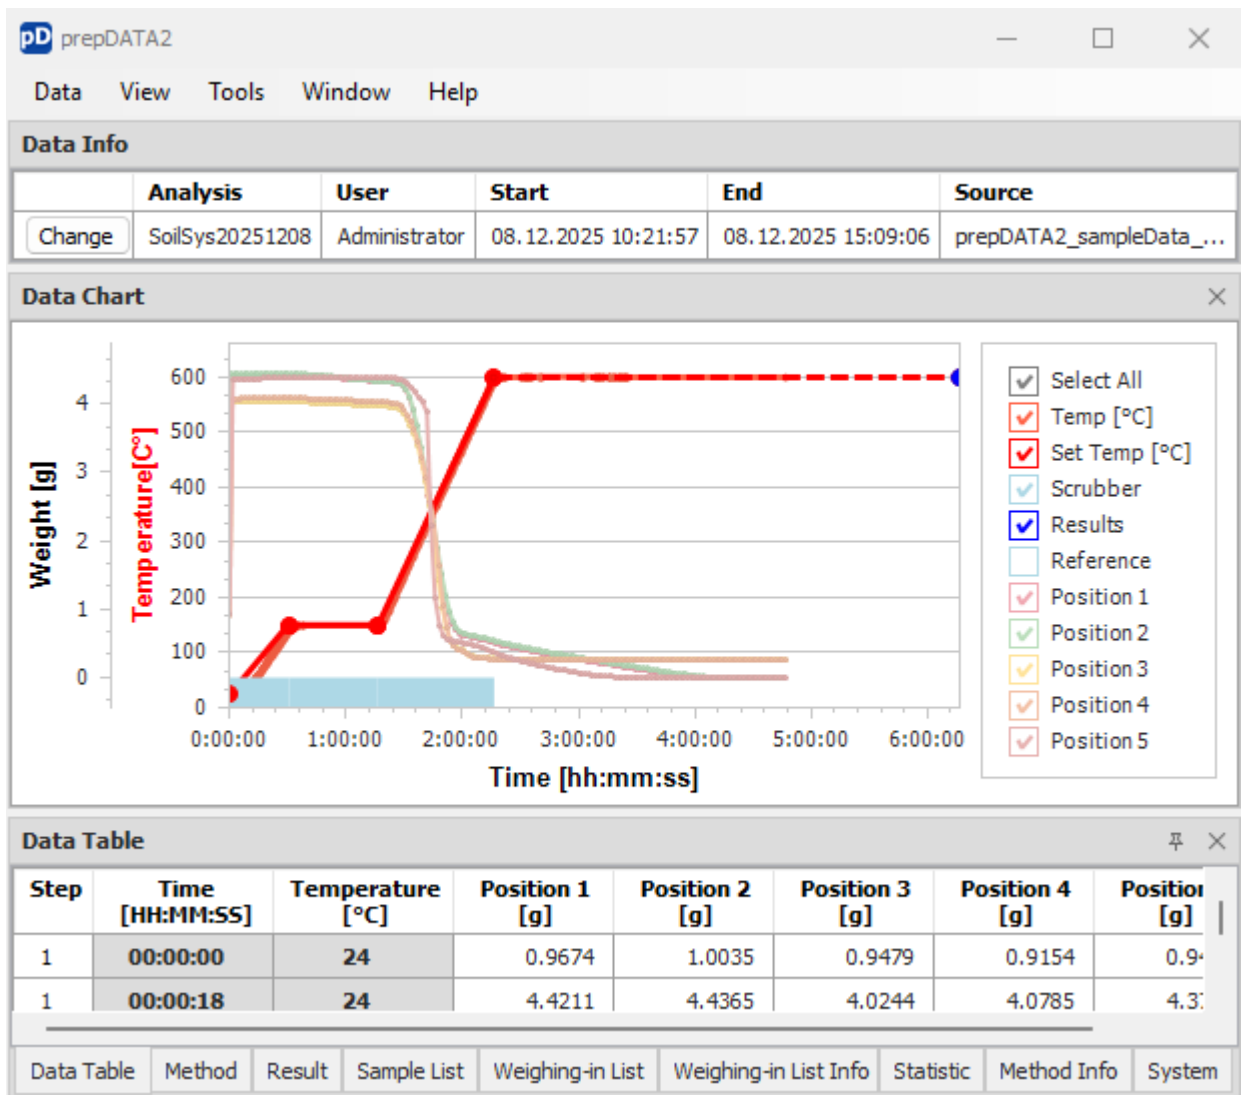

4. Open Data from prepASH


To open data from prepASH, go to the **Data** menu and select **Open from prepASH**.

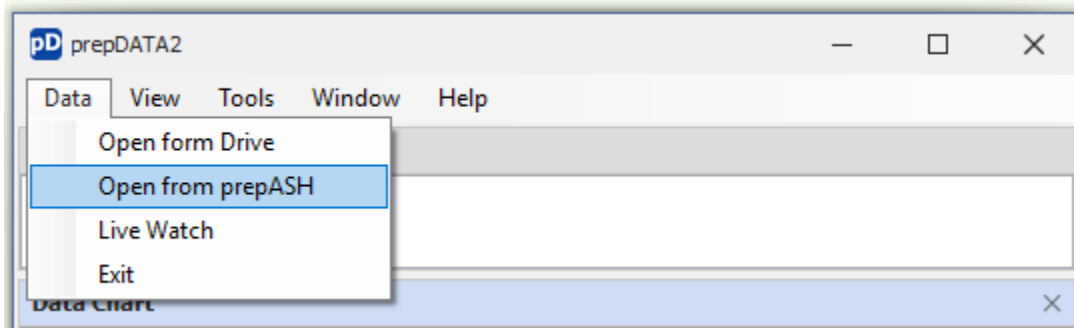


The Open from prepASH window is displayed.

4.1 Select prepASH

In the Select prepASH window, click on **Search** to refresh the list of available prepASH devices. Then select a prepASH device and click on **Select**.

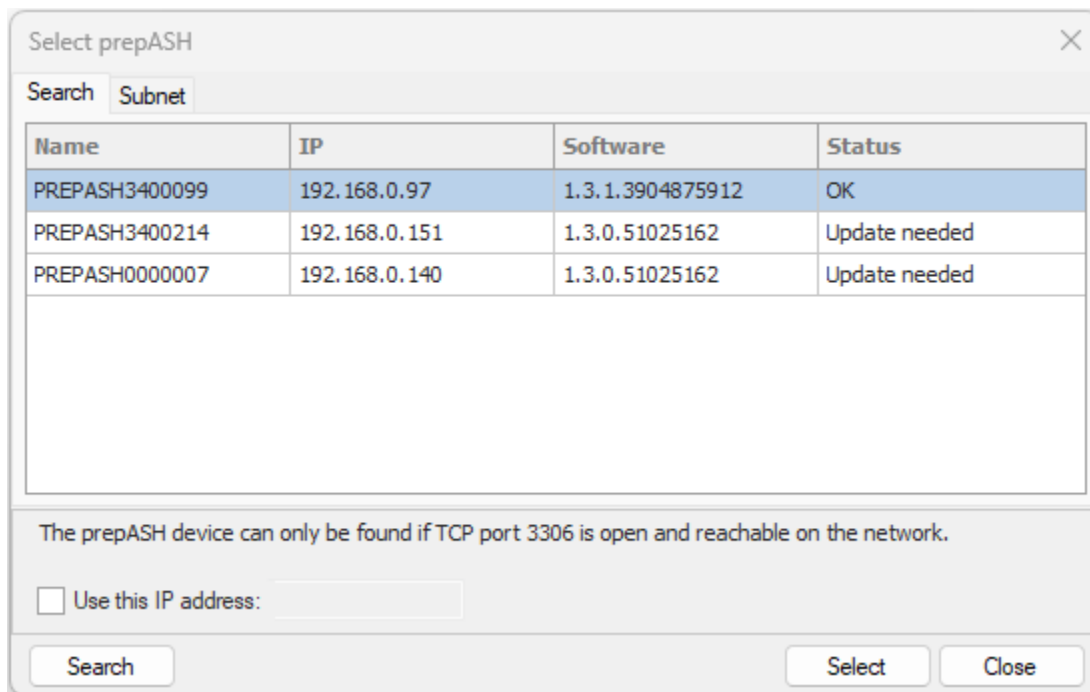


In the Subnet tab, you can add additional subnets. Your prepASH device will only be discovered if the correct Subnet is configured.

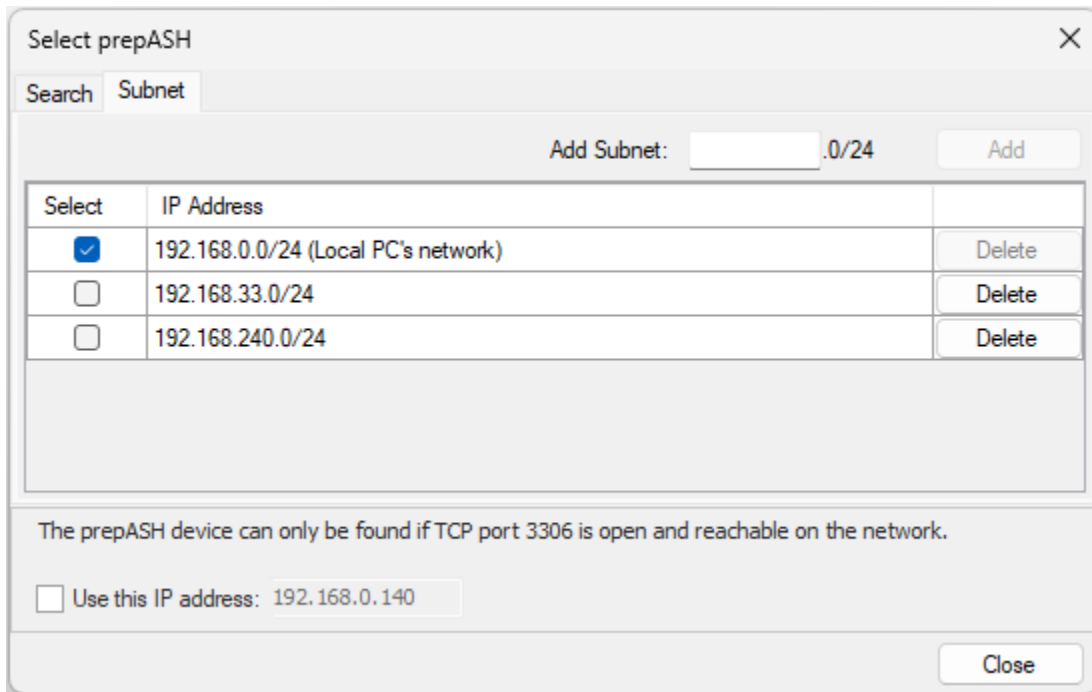

Please note that TCP port 3306 must be open and accessible on the network.
 If you encounter network issues, please contact your administrator.

4.2 Select Data

After selecting a prepASH device, a list of all available analyses is displayed.

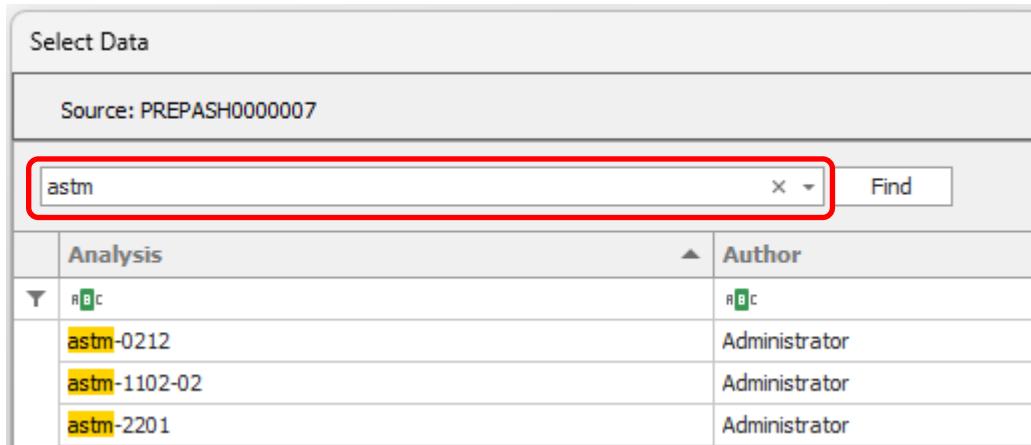


Use the “**Enter text to search...**” field to filter data across all columns, or apply filters directly under the column headers.


Select the desired analysis and click on **Select** to open it.

5. Live Watch

To open Live Watch, navigate to the **Data** menu and select **Live Watch**.

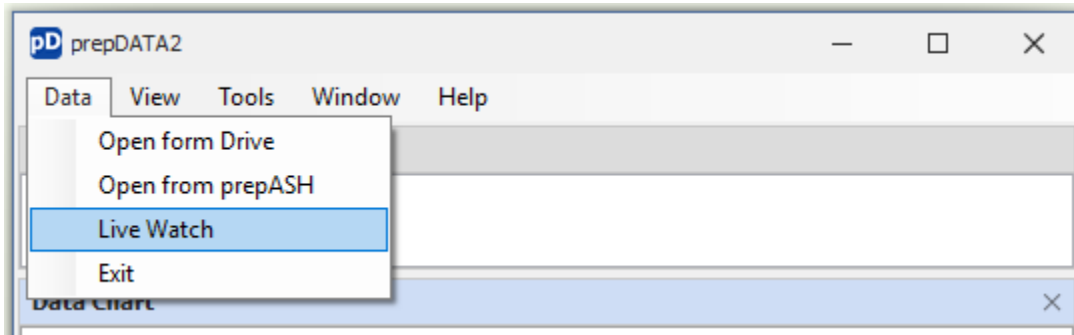

Select a prepASH device and click on **Select**.

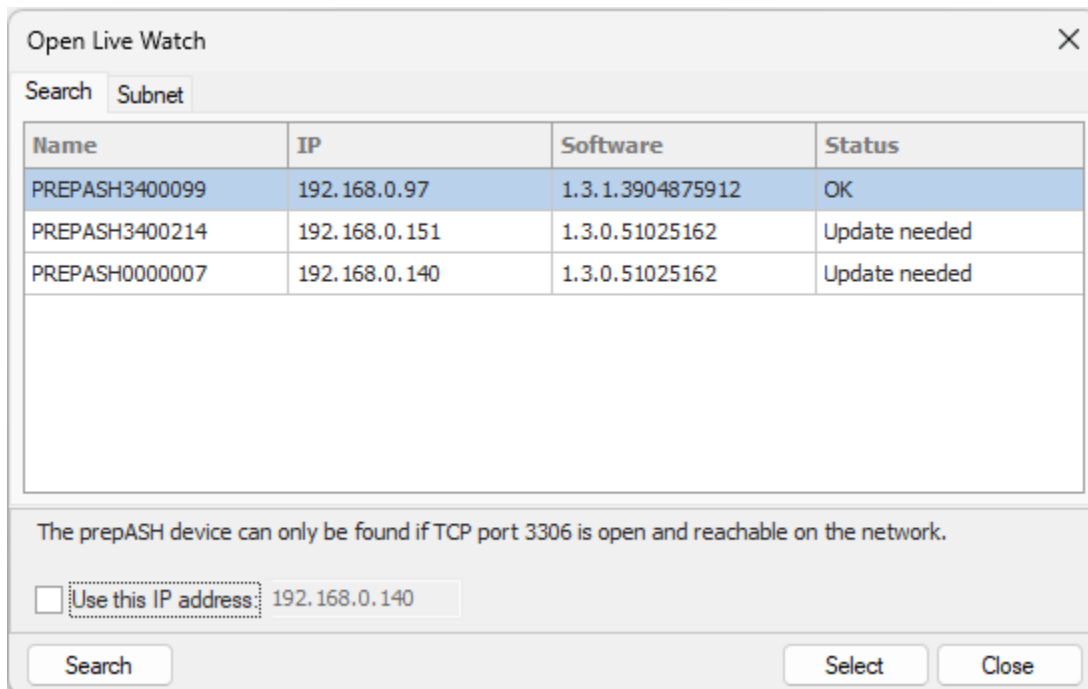


The Data Info, Data Table, and Data Chart are updated continuously.

Data Info					
	Source	Last Update	Cover	State	Temperature
LIVE	PREPASH0000007	17.07.2024 12:17:12	open	idle	25 °C

The Last update field shows when the data was last updated.


6. Chart

Ensure the Data Chart panel is visible by selecting **Data Chart** from the **View** menu.

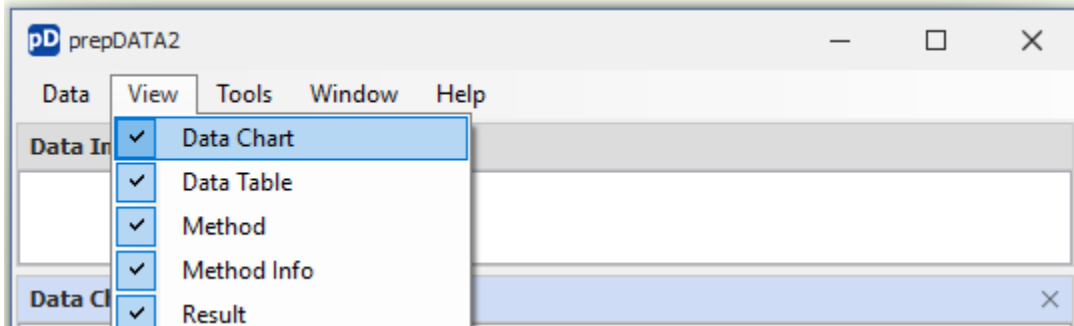


6.1 Select Samples

In the chart legend on the right side of the chart, select or deselect samples by checking the corresponding checkboxes.

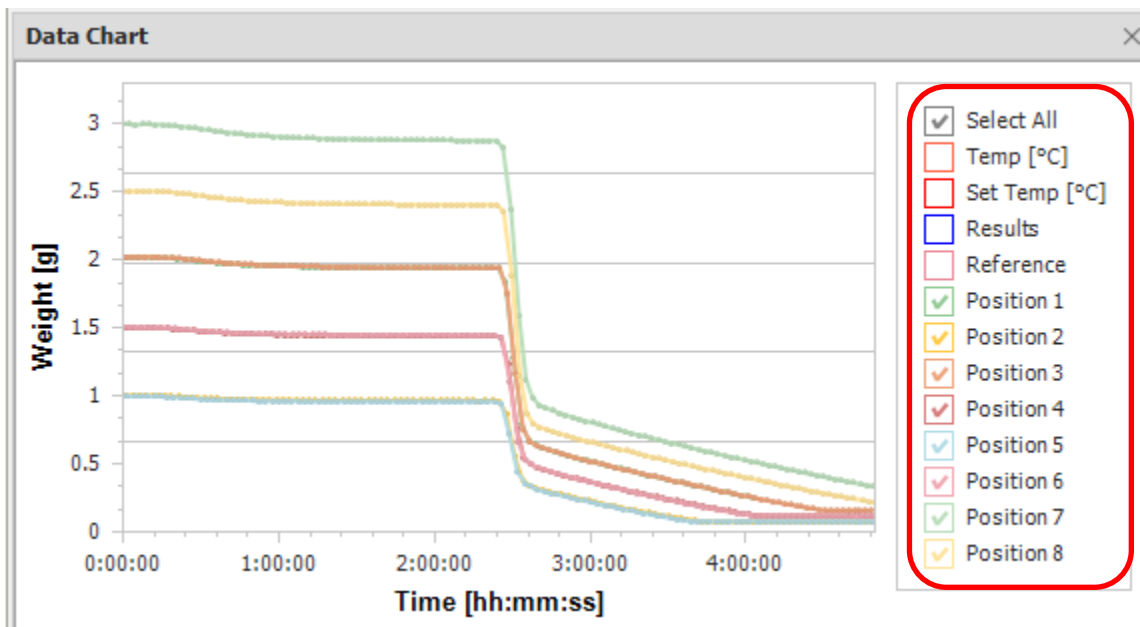


6.2 Zoom and Scroll

Press and hold the *Shift* key, then drag to select the area you want to zoom in on. Alternatively, you can zoom using the mouse scroll wheel. To scroll, click and drag within the diagram.

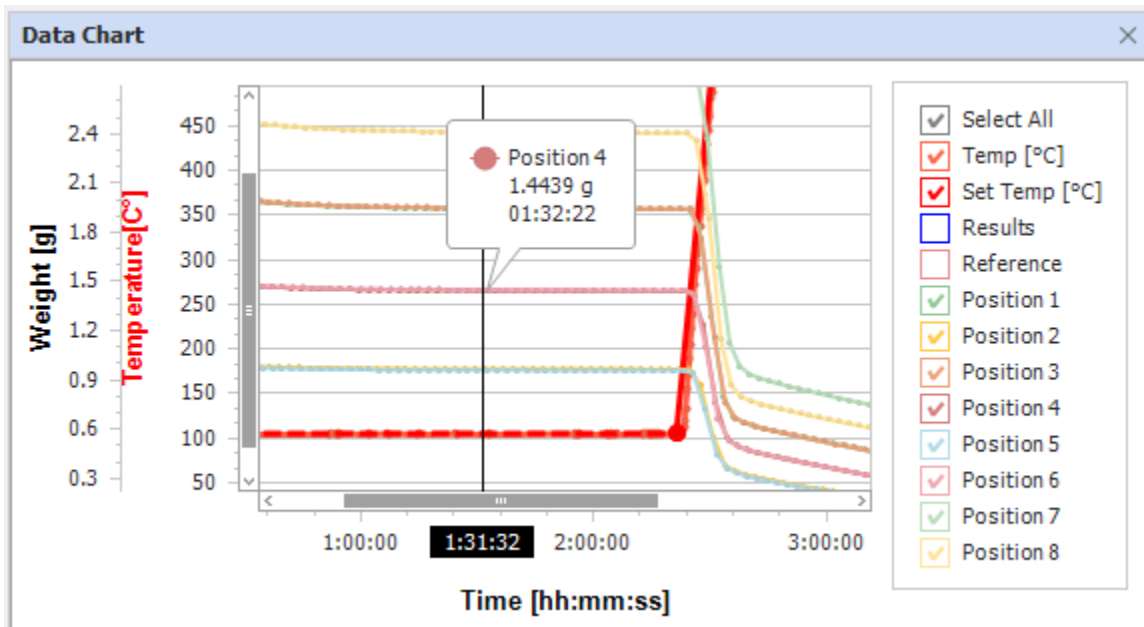

7. Result

Ensure the Result panel is visible by selecting **Result** from the **View** menu.

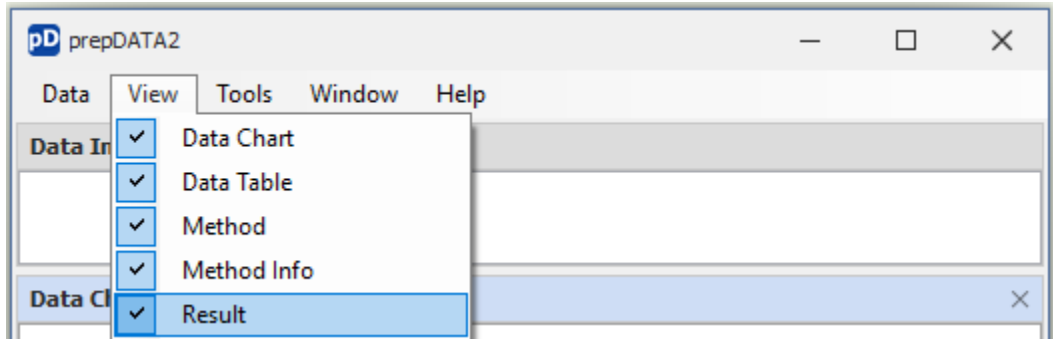

7.1 Result Editor

Click on the Result tab to display the result panel.

Result						
Method	Result Name	Calculation Mode	Unit	Step	Relative to	Calculation
<input checked="" type="checkbox"/>	R1	rest	%	2	initial	
<input checked="" type="checkbox"/>	R2	rest	%	4	W2	
<input checked="" type="checkbox"/>	R3	free	%		initial	(W4/W2)

Additional	Result Name	Calculation Mode	Unit	Step	Relative to	Calculation
<input checked="" type="checkbox"/>	LossInitialg	loss	g	2	initial	
<input checked="" type="checkbox"/>	freeResult	free	g			I-W2

At the bottom of the interface, there is a tabbed navigation bar with the following tabs: Data Table, Sample List, Weighingin List, Weighingin List Info, Method Info, Method, **Result**, Statistic, and System. The 'Result' tab is highlighted with a red box.

On the left side of the Result panel, select results by clicking the checkboxes.

Method results are displayed in the upper table, while additional results appear in the lower table. To add additional results, fill in the table cells in the lower table and select the Additional checkboxes.

Select the Free calculation mode if you want to define custom result calculations by entering the corresponding formula in the calculation field.

The following parameters are available:

I Initial Value

C Current Value

Wn Step Value, where n is a number from 1 to 15

The following basic arithmetic operations are available for the calculation field.

“+” Addition

“-” Subtraction

“*” Multiplication

“/” Division

Example formula: $C / I * 1000$

7.2 Result Table

On the right side of the Result panel, the result table is displayed.

	Pos.	Sample	ID	Tare[g]	Initial[g]	CW	AS	Result Name	R
✓	1	S		23.6412	1.7885	✓	✓	R1 R2 R3	
✓	2	S		23.6810	1.7289	X	✓	R1 R2 R3	

The first column shows whether the sample was active (✓) or not (X).

The CW column indicates whether the checkweigher was in range (✓) or not (X).


The AS column indicates whether autostop was reached (✓) or not (⚠).

The **Calculation** field displays the formula used for each result.

ne	Residue[g]	Time	Result	Unit	Rel. to	Calculation
:00:00	0.9228	01:49:12	7.609	%	initial	$(I-D)/I*100$
:00:00	0.5203	02:34:30	40.551	%	initial	$(D-V)/I*100*X$
:00:00	0.0632	05:18:51	6.328	%	initial	$A/I*100$
			45.512	%		$100-(I-D)/I*100-(D-V)/I*100*X-A/I*100$
:00:00	0.9852	00:46:27	1.174	%	initial	$(I-D)/I*100$
:00:00	0.7886	02:34:40	21.437	%	initial	$(D-V)/I*100*X$

8. Statistic

Ensure the Statistic panel is visible by selecting **Statistic** from the **View** menu.

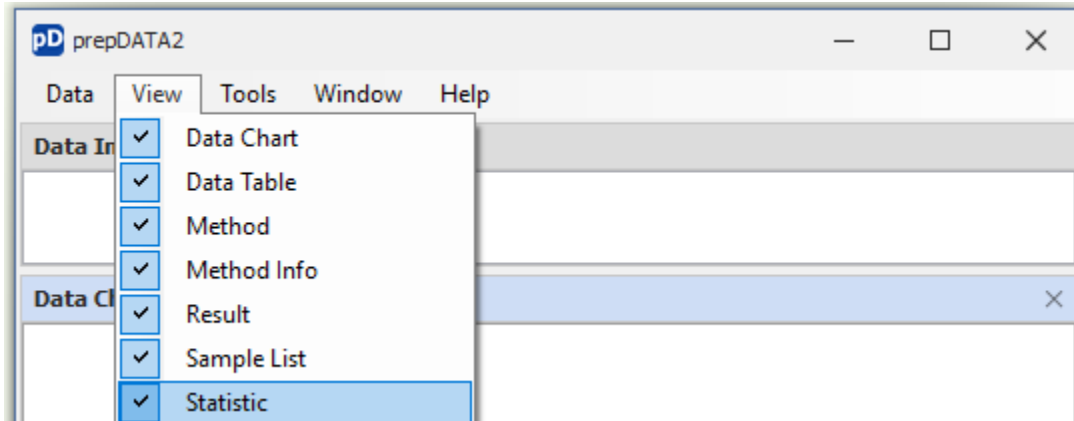

8.1 Statistic Editor

To assign the samples to groups, enter the group name in the Group field.

Statistic				
	Pos.	Sample	ID	Group
X	1			
✓	2			A
✓	3			A
✓	4			B
✓	5			B
✓	6			A
✓	7			A
✓	8			B

8.2 Statistic Table

For the values **Initial**, **Residue**, and **Result**, statistics are calculated by group

Group: A									
Result Name	Pos.	n		Initial		Residue		Result	
R1	2,3,6,7	4	mean	1.88378	g	1.80998	g	96.12275	%
			std	0.85241	g	0.81678	g	0.12031	%
			rstd	45.25014	%	45.12647	%	0.12516	%
R2	2,3,6,7	4	mean	1.88378	g	0.17970	g	9.26300	%
			std	0.85241	g	0.12718	g	2.25936	%
			rstd	45.25014	%	70.77287	%	24.39127	%
R3	2,3,6,7	4	mean					0.09250	%
			std					0.02300	%
			rstd					24.86486	%
Group: B									
Result Name	Pos.	n		Initial		Residue		Result	
R1	4,5,8	3	mean	1.66860	g	1.60267	g	96.08733	%
			std	0.76837	g	0.73574	g	0.13220	%
			rstd	46.04860	%	45.90748	%	0.13758	%
R2	4,5,8	3	mean	1.66860	g	0.14667	g	8.81400	%
			std	0.76837	g	0.08695	g	1.17091	%
			rstd	46.04860	%	59.28574	%	13.28465	%
R3	4,5,8	3	mean					0.08800	%
			std					0.01212	%
			rstd					13.77768	%

The following calculations are performed.


$$\text{mean: } \bar{x} = \frac{\sum_{i=1}^n x_i}{n}$$

$$\text{std: } s = \sqrt{\frac{1}{N-1} \sum_{i=1}^N (x_i - \bar{x})^2} \quad \text{Standard Deviation}$$


$$\text{rstd: } rstd = \frac{std}{\bar{x}} \cdot 100\% \quad \text{Relative Standard Deviation}$$

9. Export to Excel

To export data to Excel, open the **Tools** menu and choose **Export to Excel**.

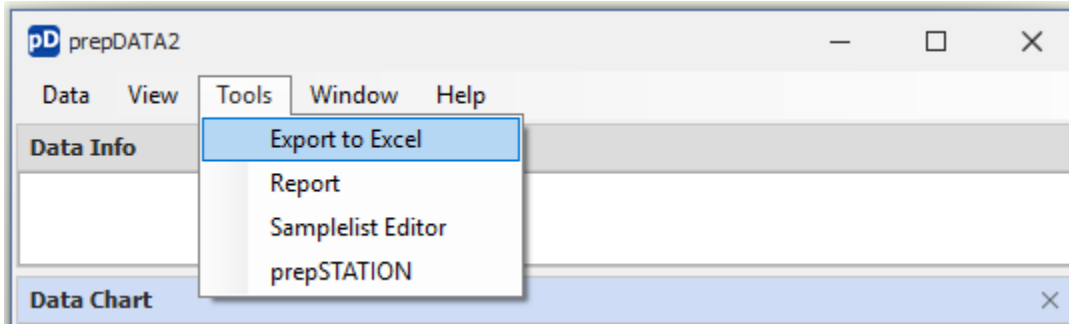

A file dialog opens. Select the file name and the folder where the export file should be saved, then click on **Save**.

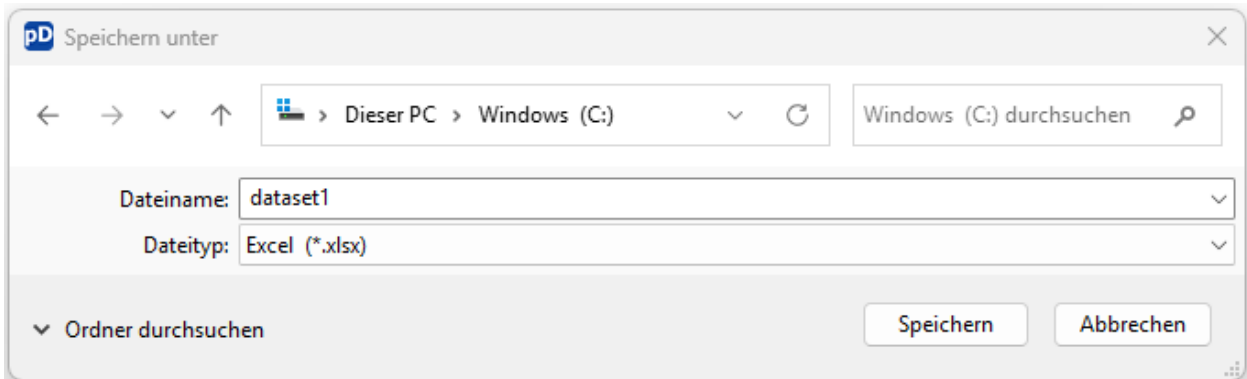


All tables are exported to the Excel file in the corresponding tabs.

	A	B	C	D	E	
1	Step	Time [HH:MM:SS]	Temperature [°C]	Reference [g]	Position 1 [g]	Positic
2	1	00:00:00	19	20.1578	2.0206	1.0045
3	1	00:00:18	19	20.1587	2.0201	1.0042
4	1	00:02:50	19	20.1586	2.0201	1.0043

Below the table, the Excel tabs are visible: 'Data Info', 'Data' (selected), 'Samplelist Info', 'Samplelist', 'Weighinglist', and 'Me'.


10. Report

To create a report, open the **Tools** menu and choose **Report**.

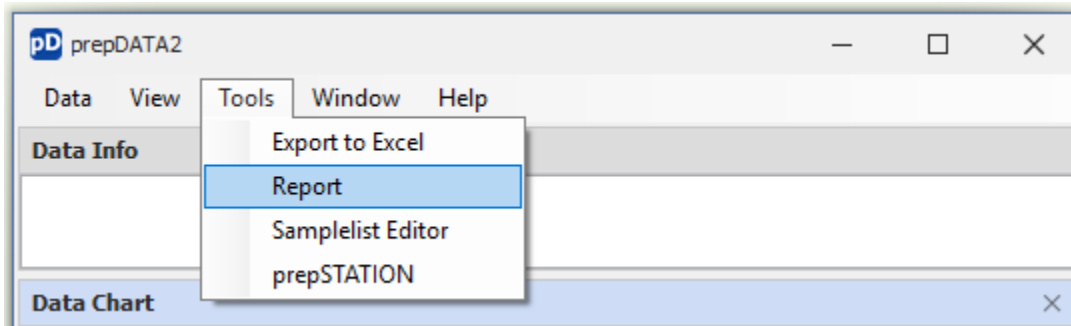


A Report Window opens where you can customize the report.

Open the **Custom Report** dropdown menu and select the desired sections by checking the checkboxes.

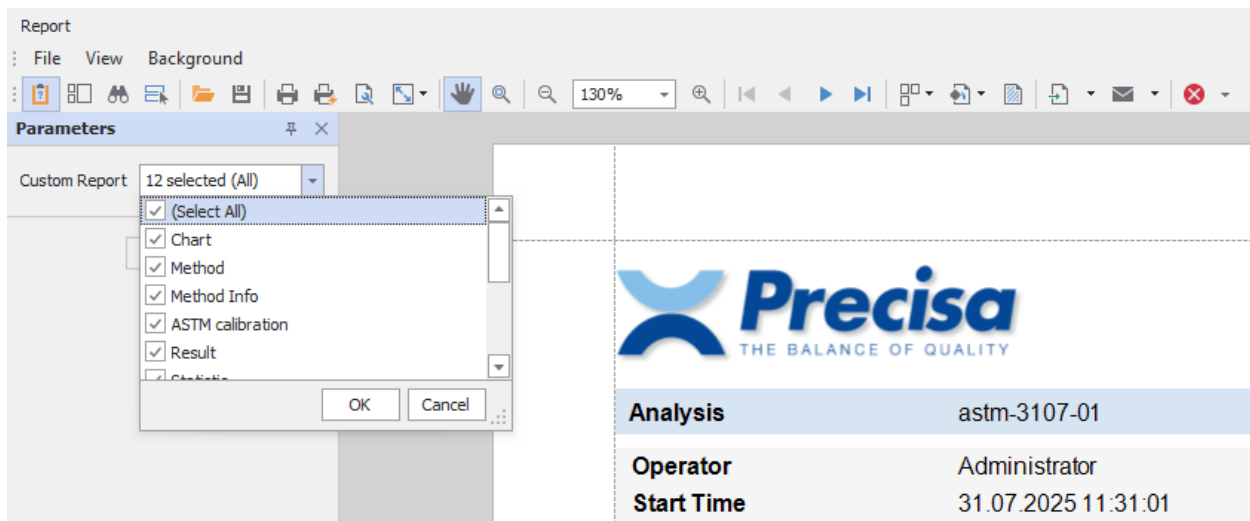


Click on **Submit** to apply the changes.

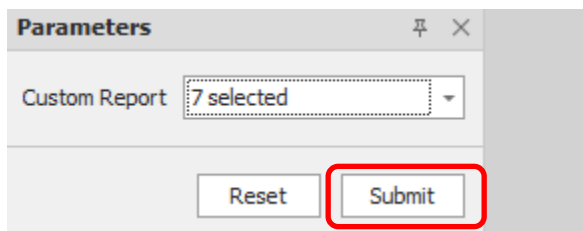


11. Samplelist Editor

To create a sample list, open the **Tools** menu and choose **Samplelist Editor**.

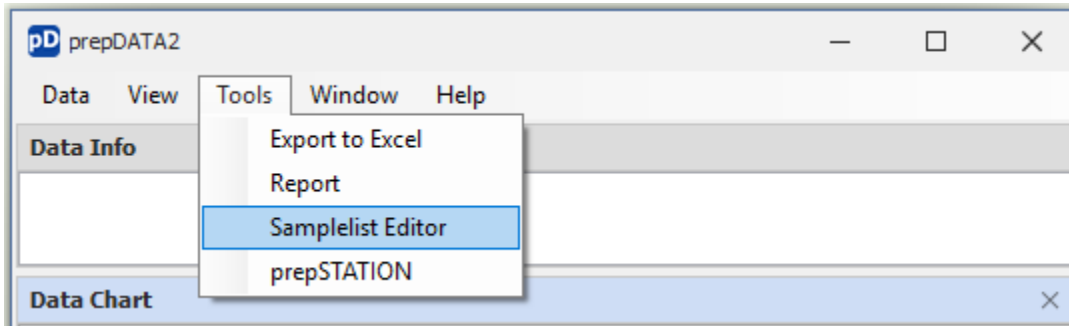


11.1 Create new Samplelist

Create a new sample list by editing the table. Use the **Select** checkboxes to include or exclude each entry. To reset the table, click on **Clear**.

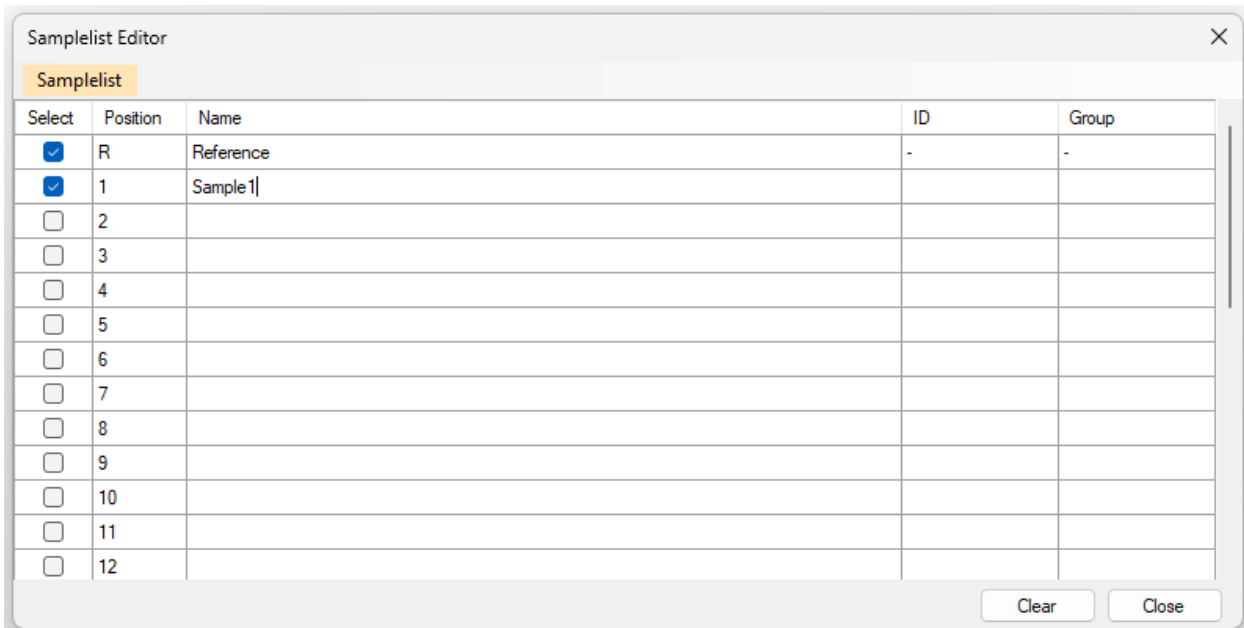


11.2 Export Samplelist

To export a sample list, open the **Samplelist** menu and select **Export**.

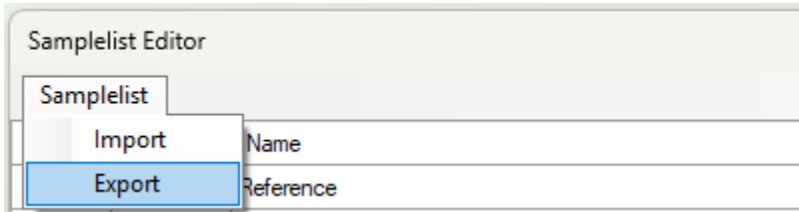


1. Use the drop-down menu to select prepASH or drive.
2. Click on **Select** to choose a prepASH device or a file.
3. Click on **Edit** to set the author.
4. Click on **Edit** to set the list name.
5. Click on **Export** to export the sample list.

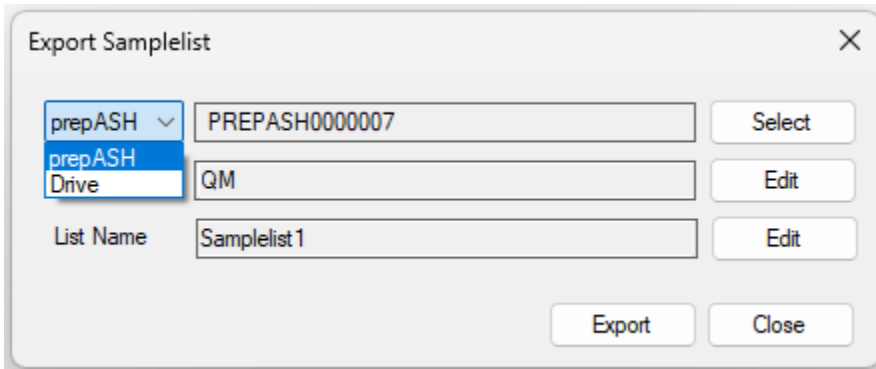


11.3 Import Samplelist

To import a sample list, open the **Samplelist** menu and select **Import**.

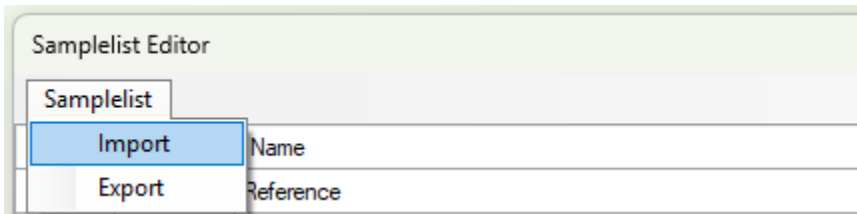


1. Use the drop-down menu to select prepASH or Drive.
2. Click on **Select** to choose a prepASH device or a file.
3. Click on **Select** to choose a sample list.
4. Click on **Import** to import the sample list.

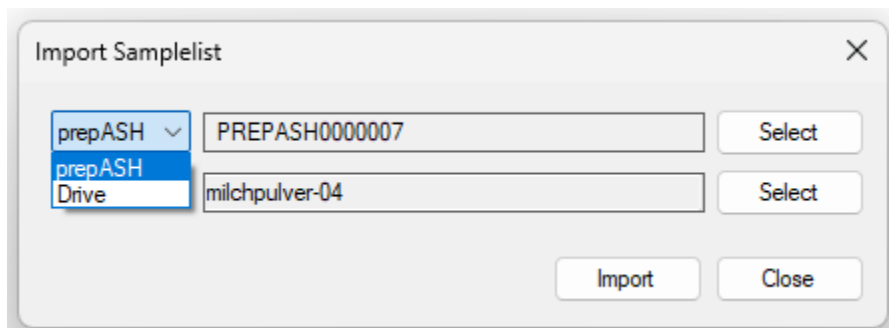


12. prepSTATION 2.0


To create a weighing-in list, the prepSTATION 2.0 (order no. 340-9011) is required, which consists of the rotary unit and a PB 120A analytical balance.

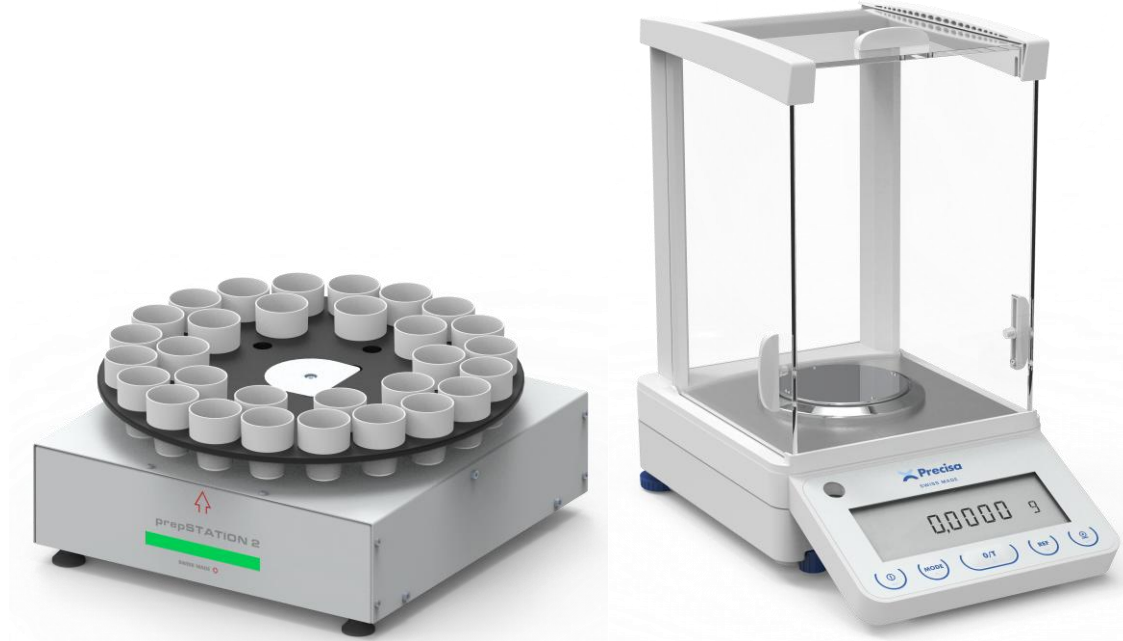

To create a weighing-in list, open the **Tools** menu and choose **prepSTATION**.

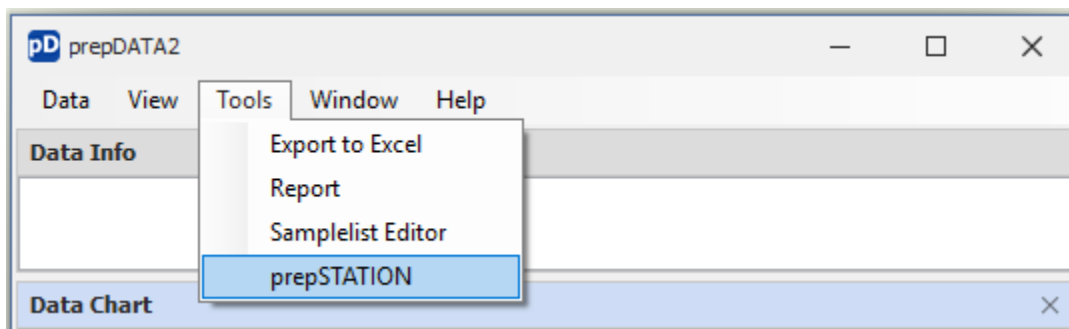


The prepSTATION window is displayed.

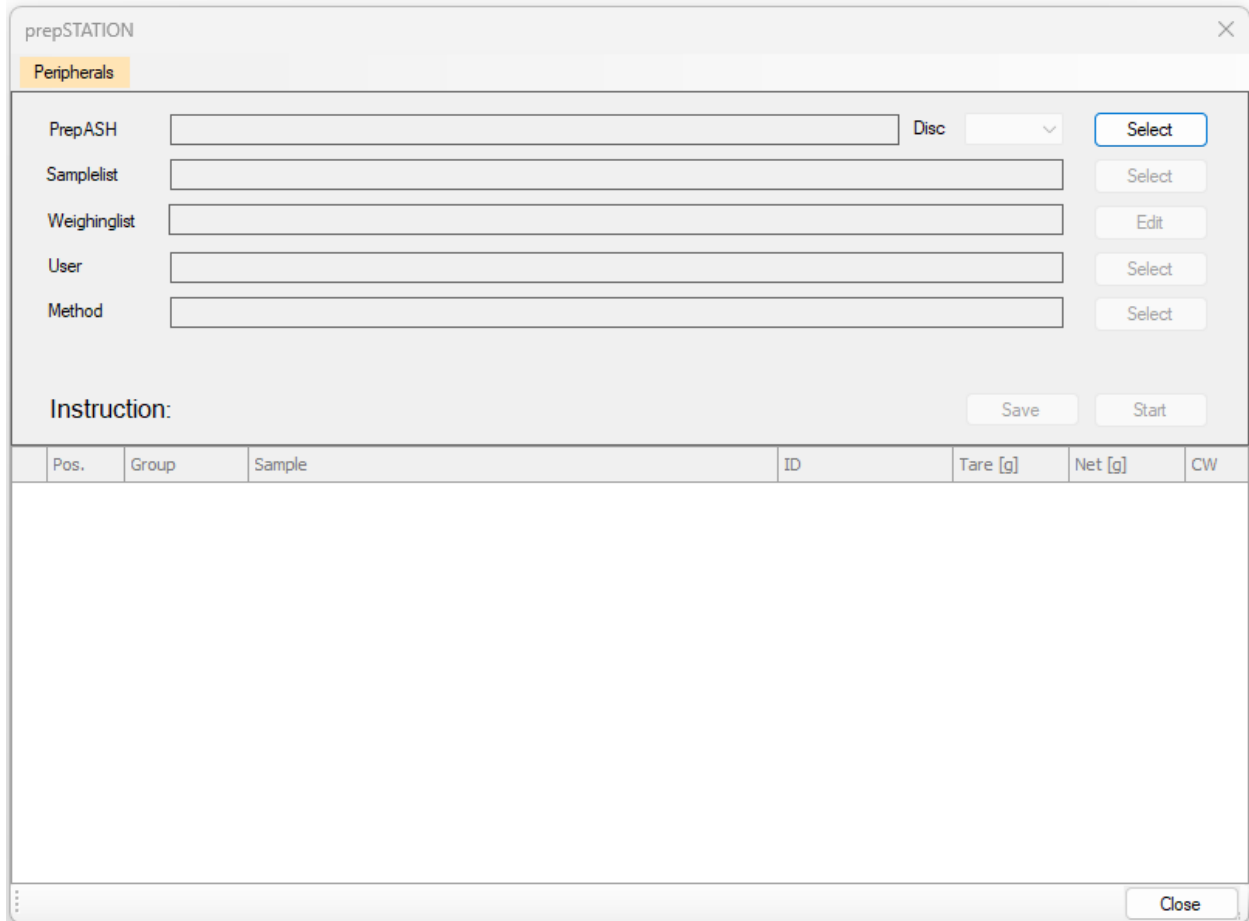


When using the prepSTATION for the first time, you need to set up the peripherals.

12.1 Setup the Balance

Open the **Peripherals** menu and select **Balance**.

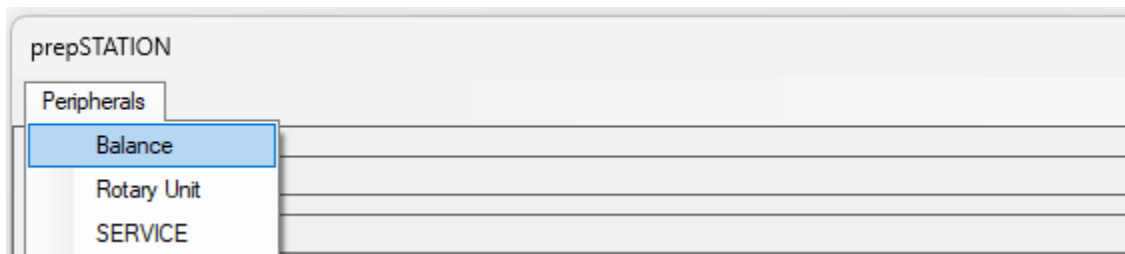

The Select Balance window is displayed.

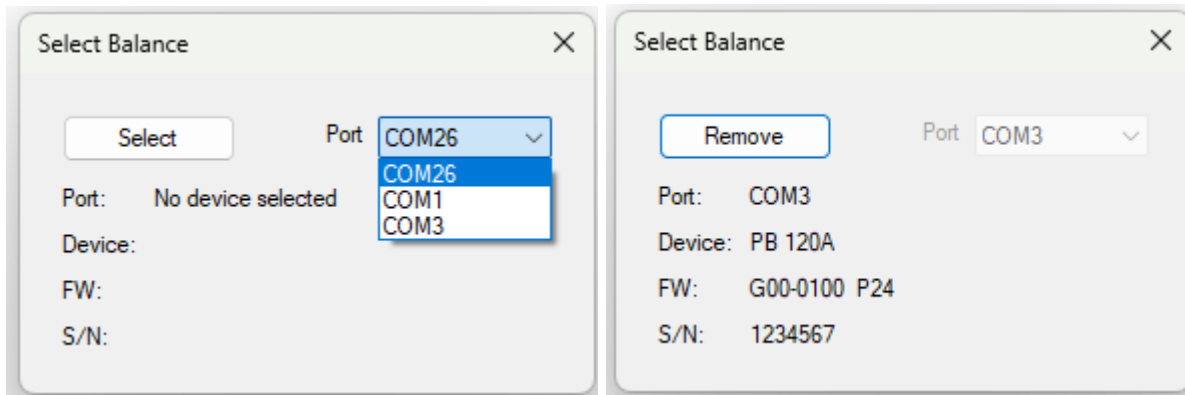


Connect the balance to the PC using a USB cable. Then select the COM port and click on **Select**. If the device is detected and ready for use, the firmware version and serial number are displayed. Close the window by clicking the **X** icon.

Hint


The serial port of the balance must be configured to **9600 baud, 8 data bits, no parity**.

12.2 Setup the Rotary Unit

Open the **Peripherals** menu and select **Rotary Unit**.

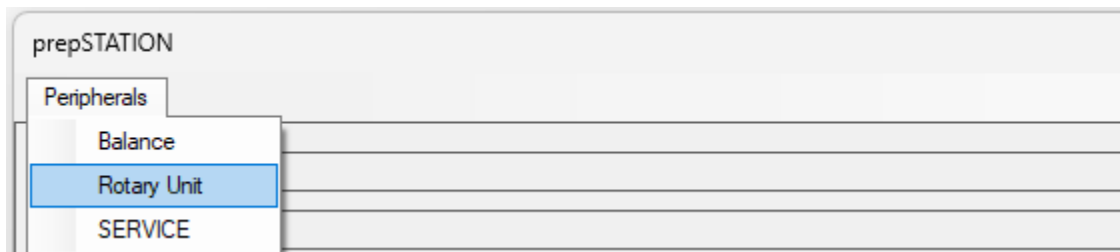


The Select Rotary Unit window is displayed.

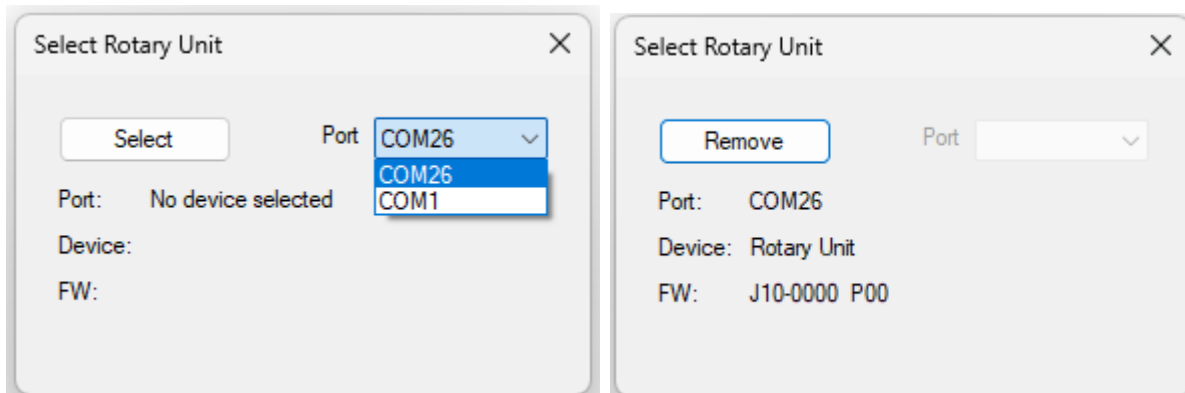

Connect the rotary unit to the PC using the USB cable. Then select the COM port and click on **Select**. If the device is detected and ready for use, the firmware version will be displayed. Close the window by clicking the **X** icon.


12.3 Adjusting the Rotary Unit

Open the **Peripherals** menu and select **SERVICE**.

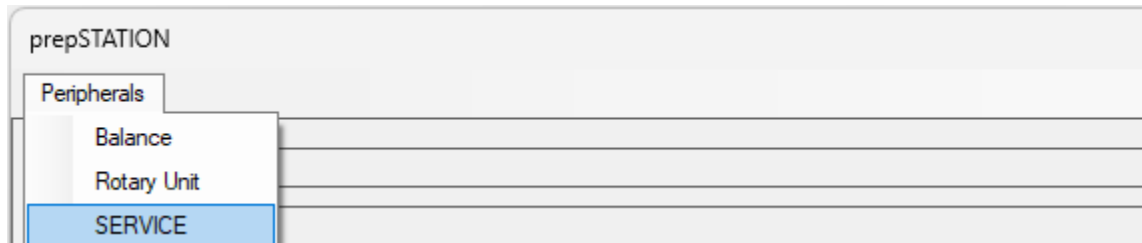

The Service window is displayed.

To adjust the reference position, follow the procedure described in the “**Set Reference**” section.

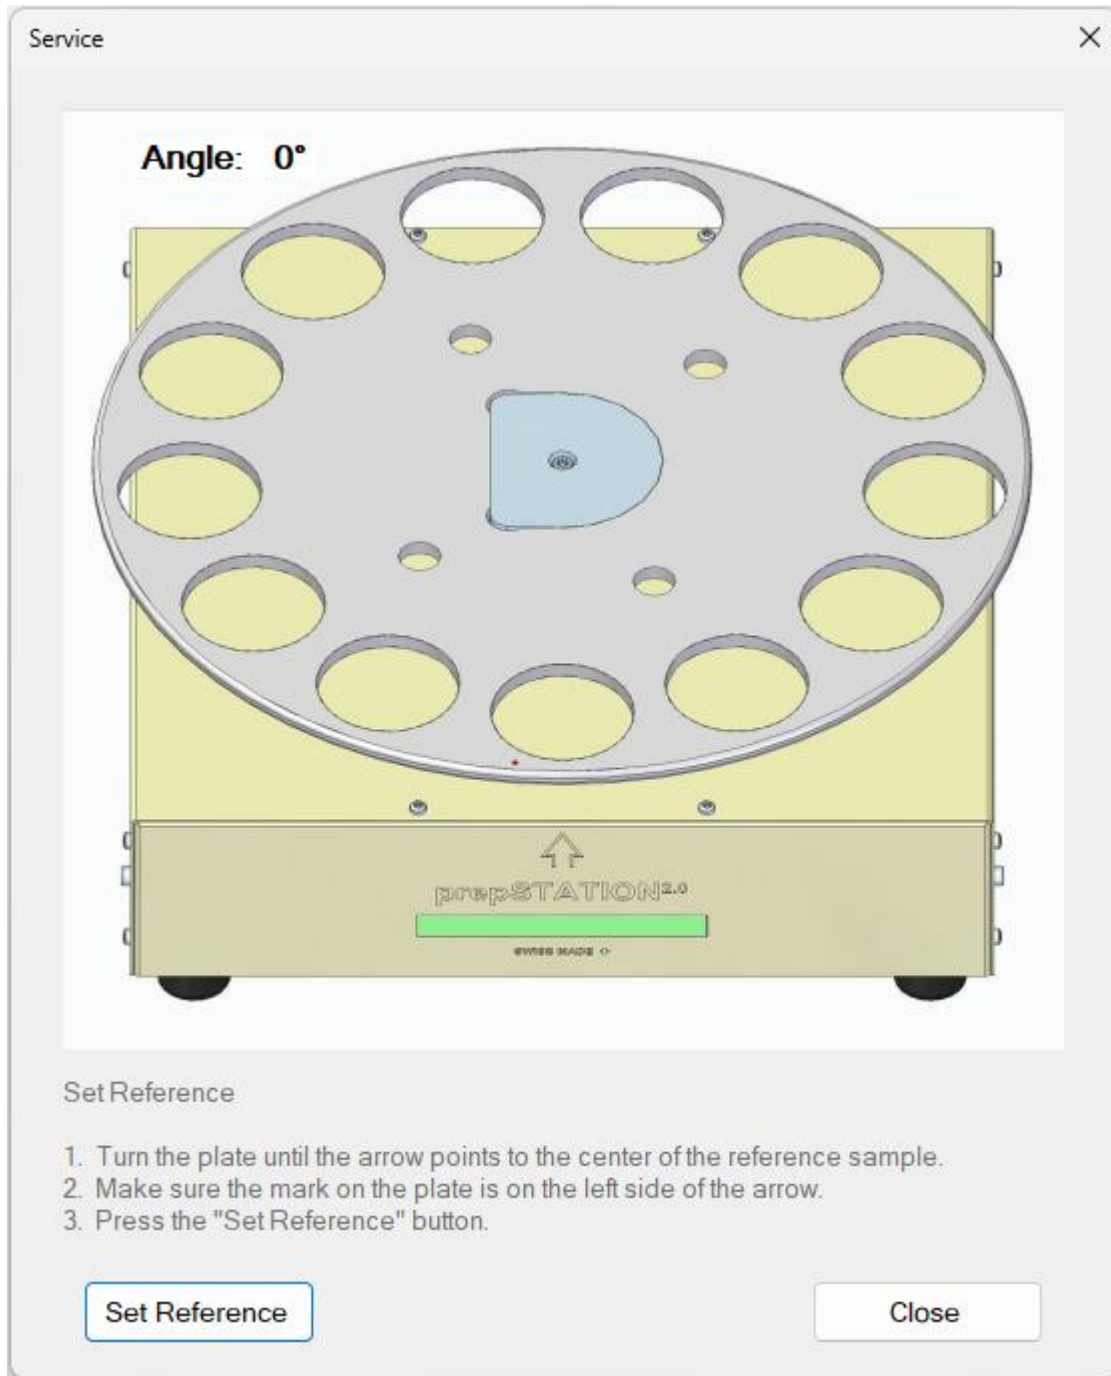

12.4 Weighing-in

1. Click on **Select** to choose a prepASH to start.

prepSTATION

Peripherals

PrepASH: PREPASH0000001 Sample plate: 29

Sample list: Samplelist 1

Weighing-in list: Weighing-in list 1

User: Administrator

Method: checkweigher

Checkweigher: On Nominal: 10.5555 g Tolerance: 1 %

Buttons: Save, Start, Select (highlighted), Select, Edit, Select, Select

Pos.	Group	Sample	ID	Tare [g]	Net [g]	CW
R	-	Reference	-			
1		Sample 1				

Close

The Select prepASH window is displayed. Select a prepASH device and click on **Select**.

Select prepASH

Search Subnet

Name	IP	Software	Status
PREPASH3400099	192.168.0.97	1.3.1.3904875912	OK
PREPASH3400214	192.168.0.151	1.3.0.51025162	Update needed
PREPASH0000007	192.168.0.140	1.3.0.51025162	Update needed

The prepASH device can only be found if TCP port 3306 is open and reachable on the network.

Use this IP address: _____

Buttons: Search, Select, Close

2. Click on the drop-down field and select the sample plate.
3. Click on **Select** to choose a sample list.

4. Click on **Edit** to set the weighing list name.
5. Click on **Select** to select the user.
6. Click on **Select** to select the method.
7. Click on **Start**.

Follow the on-screen instructions to perform the weighing.

prepSTATION

Peripherals

PrepASH: PREPASH0000001 Sample plate: 29

Sample list: Samplelist1

Weighing-in list: Weighing-in list 1

User: Administrator

Method: checkweigher

Checkweigher: On Nominal: 10.5555 g Tolerance: 1 %

Rotate plate to position <R>.

Pos.	Group	Sample	ID	Tare [g]	Net [g]	CW
R	-	Reference	-			
1		Sample 1				

When all samples have been weighed, click on **Save** to store the data on the prepASH.

prepSTATION

Peripherals

PrepASH: PREPASH0000001 Sample plate: 29

Sample list: Samplelist1

Weighing-in list: Weighing-in list 1

User: Administrator

Method: checkweigher


Checkweigher: On Nominal: 10.5555 g Tolerance: 1 %

Weighing complete.

Pos.	Group	Sample	ID	Tare [g]	Net [g]	CW
R	-	Reference	-	15.7113	15.7113	
1		Sample 1		15.7109	10.4928	✓

13. Audit Trail Viewer


To start the audit trail viewer, open the **Tools** menu and choose **Audit Trail Viewer**.

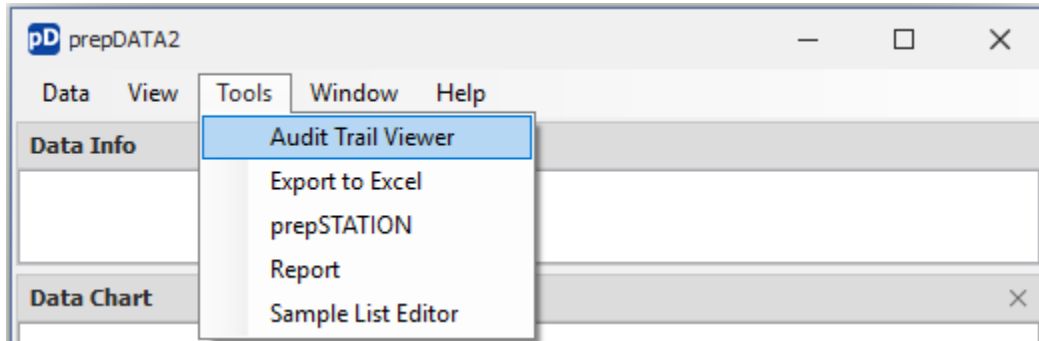


The Audit Trail Viewer window is displayed.

13.1 Import

Open the **Audit Trail** menu and select **Import**.

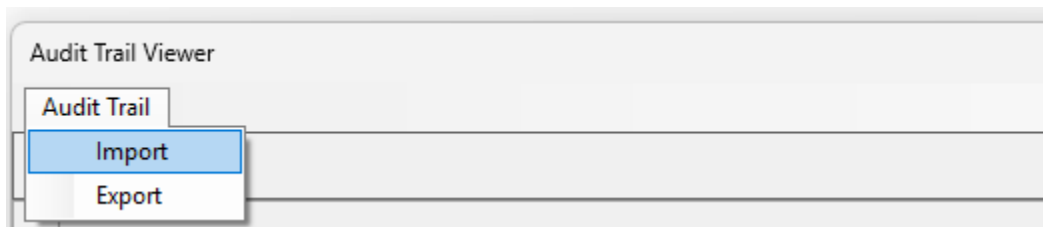


1. Use the drop-down menu to select prepASH or Drive.
2. Click on **Select** to choose a prepASH device or a file.
3. Click on **Import** to import the audit trail.

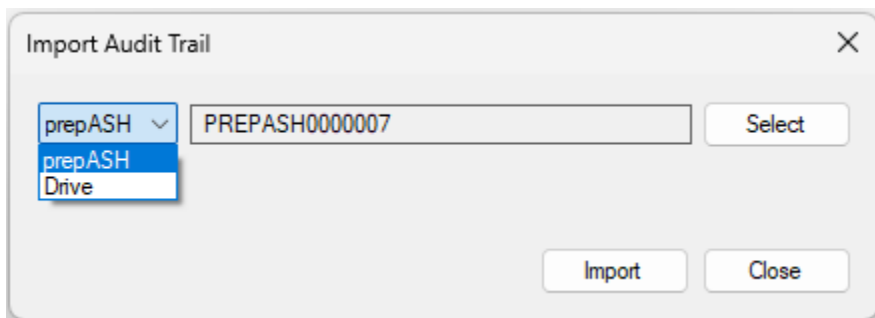


13.2 Export

Open the **Audit Trail** menu and select **Export**.

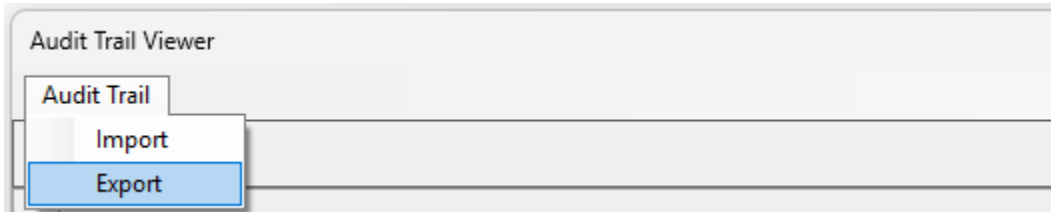


In the Export to Drive window, choose a location, enter a filename and then click on **Save**.

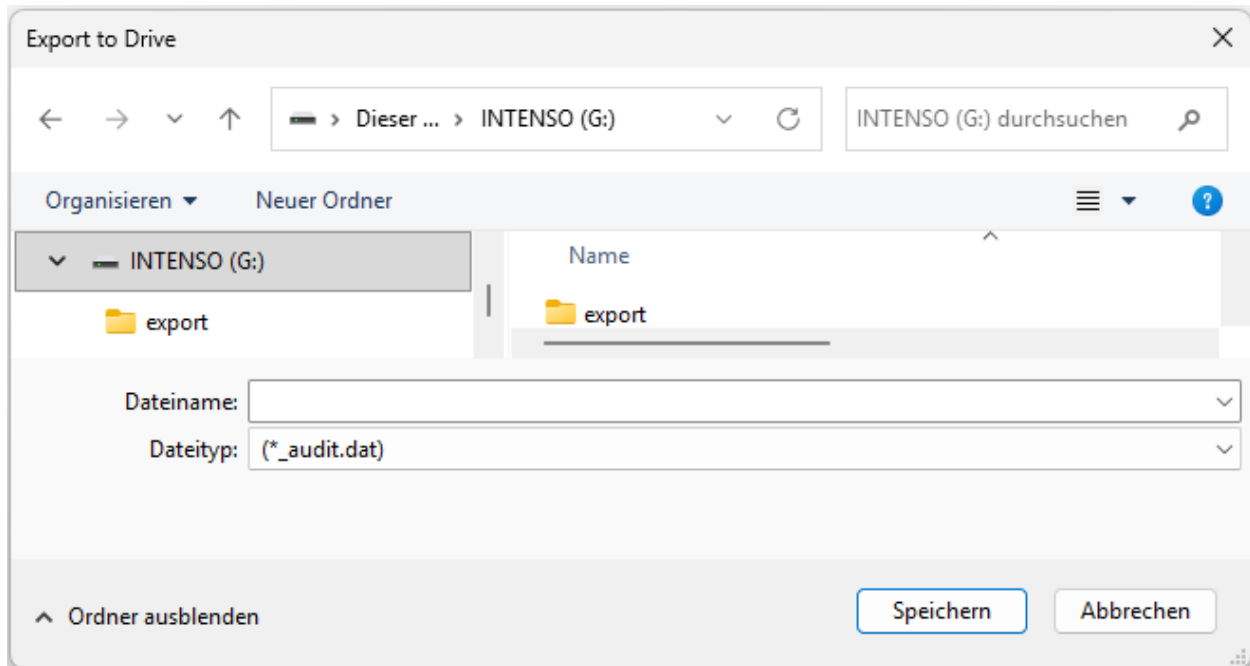

13.3 Filtering

Type your search term directly into the filter field at the top. The table updates automatically and displays only matching entries.

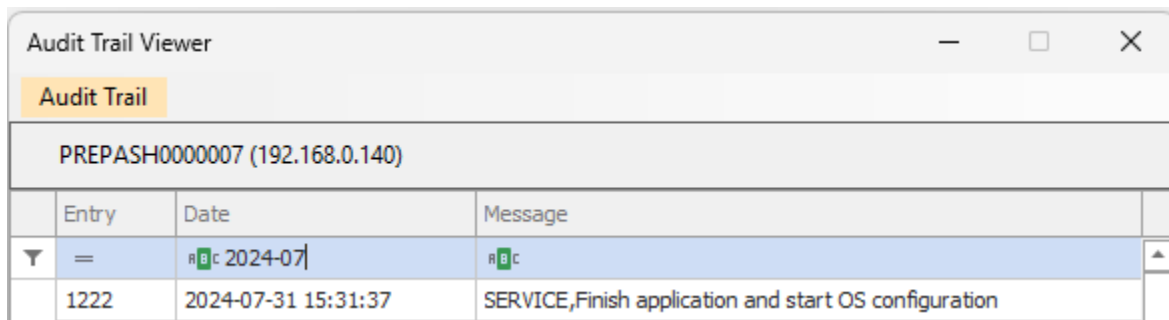

Select the first entry you are interested in. Then remove the filter by clicking the red cross.

1152	2024-07-03 13:16:13	System,Power blackout,Ended
1153	2024-07-03 13:33:03	System,Power blackout,Occurred
1154	2024-07-03 13:38:27	System,Power blackout,Ended

× Date Contains 2024-07

The selected row stays marked and you can scroll through the nearby entries.

Audit Trail

PREPASH0000007 (192.168.0.140)

Entry	Date	Message
▼ =	⌘	⌘
1204	2024-07-25 14:58:48	Administrator,Service button pressed
1205	2024-07-25 15:00:03	SERVICE,Finish application and start OS configuration
1206	2024-07-25 16:49:03	System,Service button pressed
1207	2024-07-25 16:51:23	SERVICE,Finish application and start OS configuration
1208	2024-07-31 08:42:00	System,Service button pressed
1209	2024-07-31 08:44:35	SERVICE,Finish application and start OS configuration
▶ 1210	2024-07-31 09:11:26	Administrator,Login,
1211	2024-07-31 09:12:23	Administrator ,Logout
1212	2024-07-31 09:12:56	Administrator,Login,
1213	2024-07-31 09:13:24	Administrator ,Logout
1214	2024-07-31 14:02:21	Administrator,Login,
1215	2024-07-31 14:02:27	Administrator,Start application,Import/Export
1216	2024-07-31 14:06:17	Administrator,Analysis,Export
1217	2024-07-31 14:06:50	Administrator,Analysis,Export
1218	2024-07-31 14:07:04	Administrator ,Logout
1219	2024-07-31 15:26:54	Administrator.Login.